





(Electronic version)

<sub>1コ1号 ド</sub>载报告



VERIFICATION WEBSITE: www.gttc.net.cn VERIFICATION CODE: TKSO-0712-24

ISSUE DATE: 2020-04-13

APPLICANT: ZHAOQING BOHAN SPORTS CO., LTD

NO. 2-1, KANG TAI STREET, HIGH-TEC ZONE, ZHAOQING CITY, GUANGDONG, CHINA ADDRESS:

SAMPLE INFORMATION:

FORTY FOLDING PARTICULATE PROTECTIVE MASKS

BRAND: KOUMASK

STYLE NO.: 20200315

COLOUR: WHITE SIZE: KKF-1A

MANUFACTURE'S NAME: ZHAOQING BOHAN SPORTS CO., LTD

| DATE RECEIVED/DATE TEST STARTED: 2020-04-03  |   |
|--|---|
| CONCLUSION:  |   |
| FILTRATION EFFICIENCY TO NaC1 PARTICULATE MATTER                                     | M |
| INSPIRATORY RESISTANCE   | M |
| EXPIRATORY RESISTANCE  | M |
| FLAMMABILITY   | M |
| HEAD BAND  | M |
| NOTE "M" MEET THE CTANDADD'S DECHIDEMENT "E" DATE TO MEET THE CTANDADD'S DECHIDEMENT |   |

"M" -MEET THE STANDARD'S REQUIREMENT "F" -FAIL TO MEET THE STANDARD'S REQUIREMENT "---" -NO COMMENT NOTE:

#### REMARK:

THIS REPORT IS THE ENGLISH TRANSLATION VERSION OF THE REPORT 200056882.

ALL THE TESTED ITEMS ARE TESTED UNDER THE STANDARD CONDITION (EXCEPT FOR INDICATION).

COPIES OF THE REPORT ARE VALID ONLY RE-STAMPED.

THE EXPERIMENT WAS CARRIED OUT AT No. 1, ZHUJIANG ROAD, PANYU DISTRICT, GUANGZHOU, GUANGDONG, P. R. CHINA.

APPROVED BY:

ZiShan Guo SENIOR ENGINEER

郭子山



总部:广州市番禺区珠江路1号

花都实验室:广州市花都区狮岭镇旗岭河滨西路1号








(Electronic version)

No: 200056883

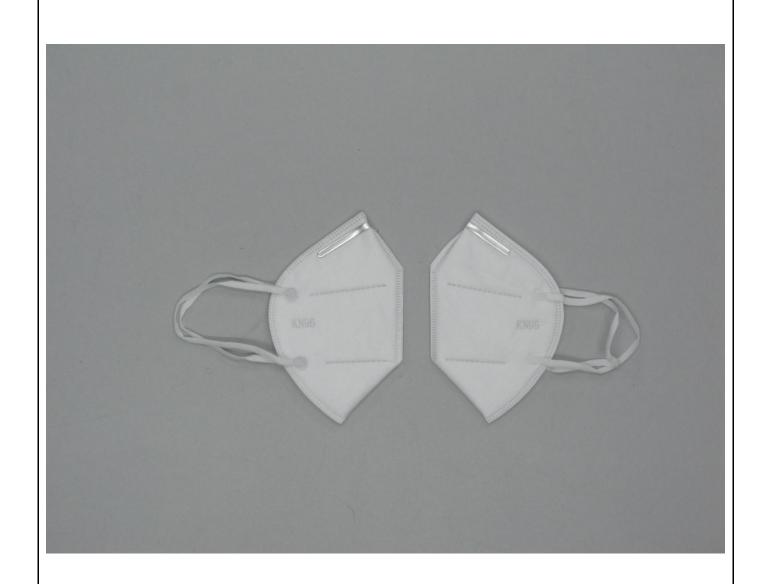

总部:广州市番禺区珠江路1号

花都实验室:广州市花都区狮岭镇旗岭河滨西路1号







(Electronic version)

No: 200056883

#### FILTRATION EFFICIENCY TO NaC1 PARTICULATE MATTER

(GB 2626-2006 6.3, AIR FLOW: 85L/min, AEROSOL: NaC1, AEROSOL CONCENTRATION:  $15 \text{mg/m}^3$ ,

TEMP: 24.3°C, RH: 38.1%)

REQUIREMENT

FILTRATION EFFICIENCY(%): FILTRATION EFFICIENCY(%):

UNTREATED SAMPLE ≥95.0 1# 99.896 (KN95)

2# 99. 980 (GB 2626-2006)

3# 99.982 (GB 2020 20

4# 99. 915 5# 99. 978

9# 99.947 10# 99.952

CONDITIONING TREATED

1# 99.910 2# 99.813

99.960

99.954

99.953

6# 7#

8#

3# 99. 947 4# 99. 890

5# 99.913

#### INSPIRATORY RESISTANCE (Pa)

(GB 2626-2006 6.5, HEAD SIZE: MEDIUM)

REQUIREMENT

UNTREATED SAMPLE: \$\leq 350\$
1\pm 103.7\$
(GB 2626-2006)

1# 103.7 2# 100.2

PRETREATMENT SAMPLE:

1# 106.0 2# 104.3

### EXPIRATORY RESISTANCE (Pa)

(GB 2626-2006 6.6, HEAD SIZE: MEDIUM)

UNTREATED SAMPLE: ≤250 1# 59.7 (GB 2626-2006)

2# 61.5

PRETREATMENT SAMPLE:

1# 61. 1 2# 58. 0

#### FLAMMABILITY(s)

(GB 2626-2006 6.15)

1# 0.0 (GB 2626-5) 2# 0.0

CONDITIONING TREATED

3# 0.0 4# 0.0



总部:广州市番禺区珠江路1号

花都实验室:广州市花都区狮岭镇旗岭河滨西路1号







(Electronic version)

No:200056883

HEAD BAND

(GB 2626-2006 6.11)

UNTREATED SAMPLE:

1# PASS

CONDITIONING TREATED:

1# PASS

REQUIREMENT

EACH HEAD BAND, BUCKLE AND OTHER ADJUST PARTS OF MASK SHOULD NOT SLIP OR BREAK UNDER 10N TENSION FOR 10S.

(GB 2626-2006)



——End of Report——

总部:广州市番禺区珠江路1号

花都实验室:广州市花都区狮岭镇旗岭河滨西路1号